REVEAL [redacted]

DOC NO: 40009 Rev: D

TITLE: RADIATION SURVEY MAP FOR CT-80, CT-80XL, CT-80DR, & CT-80DRXL

RADIATION LIMIT: < 400 µR/hr

All Readings in µR/hr unless otherwise stated

CT-80 / CT-80DR

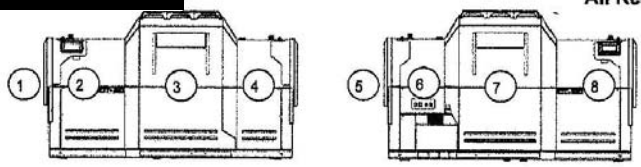

CT-80XL / CT-80DRXL

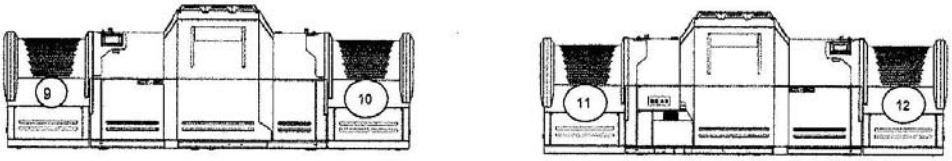

TEST RECORD

ZONE	RADIATION LEVEL VALUE (< 400 µR/hr)	ZONE	RADIATION LEVEL VALUE (< 400 µR/hr)
1) ENTRANCE END	148	5) EXIT END	109
2) RIGHT SIDE ENTRANCE TUNNEL	22	6) LEFT SIDE EXIT TUNNEL	19
3) RIGHT SIDE GANTRY	36	7) LEFT SIDE GANTRY	24
4) RIGHT SIDE EXIT TUNNEL	12	8) LEFT SIDE ENTRANCE TUNNEL	19
9) RIGHT SIDE XL ENTRANCE	N/A	11) LEFT SIDE XL EXIT	N/A
10) RIGHT SIDE XL EXIT	N/A	12) LEFT SIDE XL ENTRANCE	N/A

Technician name:	[redacted]	Date:	Mar 1, 2011
Meter Manufacturer and Model:	Thermo RadEye PRD	Unit Model and Serial Number:	CT-80 040034
Meter Serial Number:	014351	Unit Location:	BIL Airport Lobby
Meter Calibration Due Date:	May 11, 2011	Background:	6 uR/hr

Notes (Reason for Survey): Annual PM