


## CastScope Radiation Survey

Instruments required: Victoreen 451P Radiation Survey Meter, Calibrated with Cs-137

Do not substitute this survey meter! The radiation produced by CastScope is more difficult to measure than for other x-ray equipment. It is produced from a lower KV, uses a sweeping pencil beam, and is more than 500 times lower than equivalent medical examinations. In particular, meters that operate with *pulse counting* or in a *dose rate* mode will provide highly incorrect readings. The pass/fail values for this test are based on the energy response characteristics of the Victoreen 451P when calibrated with Cs-137. Other ion chambers may produce different results, depending on their energy response and calibration source. An ion chamber reading in  $\mu\text{R}$  is not the same as  $\mu\text{Rem}$  of effective dose for CastScope. Contact Spectrum San Diego for additional information before using other measurement devices.

### 1. Procedure for Direct Beam Measurement:

Set the survey meter to the integration mode, not the dose rate mode ( $\mu\text{R}$ , not  $\mu\text{R}/\text{hour}$ ). Place the meter on the face of the CastScope, as shown in the photograph. Record the initial reading on the meter. Conduct ten scans. Subtract the initial meter reading from the final meter reading and divide by ten. Record the result.

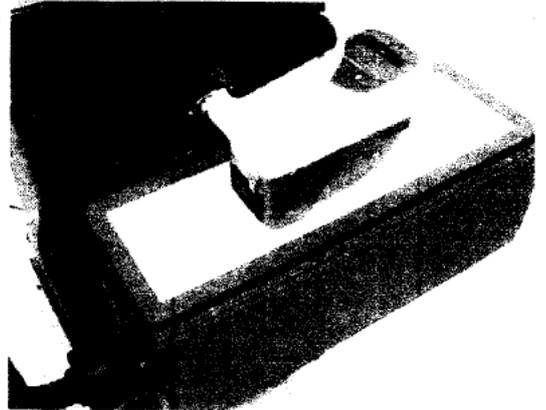

### 2. Procedure for Leakage Measurement:

Set the survey meter to the dose rate mode (i.e.,  $\mu\text{R}/\text{hour}$  or  $\text{mR}/\text{hour}$ ). Record the background measurement. Hold the meter on the back<sup>1</sup> of the imaging enclosure and conduct a scan. Repeat with the meter placed on all four sides<sup>2</sup> of the imaging enclosure. Subtract the background reading from the maximum reading. Record the result.

Date: 3-28-11

CastScope s/n 08080016

Location: TSA HEADQUARTERS JFK  
TRAINING ROOM - ROCKAWAY BLVD  
JAMAICA N.Y.

Meter s/n: 0000000513

Meter calibration date: 9/16/10

(189 ÷ 10)

1. Direct Beam Measurement: 18.9  $\mu\text{R}$   
(circle PASS if reading is less than 40  $\mu\text{R}$ , otherwise circle FAIL)

PASS FAIL

2. Leakage Measurement (Maximum-background): 0.013  $\text{mR}/\text{hour}$   
(circle PASS if reading is less than 0.25  $\text{mR}/\text{hour}$  (250  $\mu\text{R}/\text{hour}$ ), otherwise circle FAIL)

PASS FAIL

Survey conducted by: Organization: SIEMENS GOVERNMENT SERVICES (SGS)

Printed name: [REDACTED]

Signature: [REDACTED]

SSD-112-9160 Rev D, 7/31/2008

<sup>1</sup> The back side of the scan head is opposite the white direct beam exit surface

<sup>2</sup> The four sides referred to here are the 4 ones surrounding the white direct beam exit surface. Each of these sides is 90 degrees in orientation to the white direct beam surface. To more easily measure the side facing the unit, be sure to tilt the scan head on this side