REVEAL [redacted]

DOC NO: 40009 Rev: D

TITLE: RADIATION SURVEY MAP FOR CT-80, CT-80XL, CT-80DR, & CT-80DRXL

RADIATION LIMIT: < 400 µR/hr
All Readings in µR/hr unless otherwise stated

CT-80 / CT-80DR

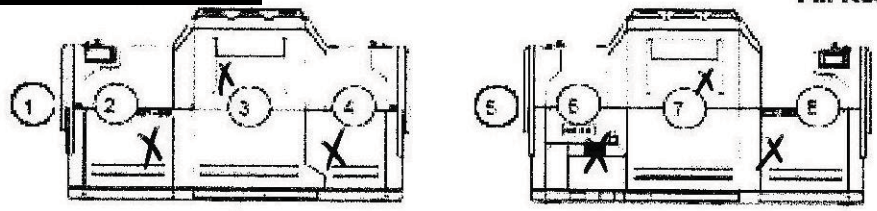

CT-80XL / CT-80DRXL

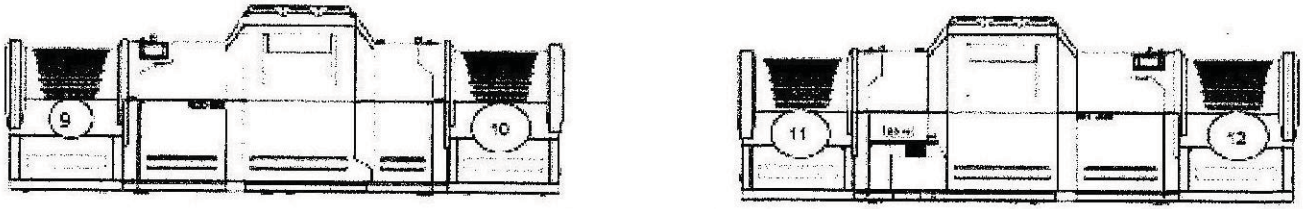

TEST RECORD

ZONE	RADIATION LEVEL VALUE (< 400 µR/hr)	ZONE	RADIATION LEVEL VALUE (< 400 µR/hr)
1) ENTRANCE END	288	5) EXIT END	359
2) RIGHT SIDE ENTRANCE TUNNEL	116	6) LEFT SIDE EXIT TUNNEL	93
3) RIGHT SIDE GANTRY	176	7) LEFT SIDE GANTRY	176
4) RIGHT SIDE EXIT TUNNEL	93	8) LEFT SIDE ENTRANCE TUNNEL	146
9) RIGHT SIDE XL ENTRANCE	n/a	11) LEFT SIDE XL EXIT	n/a
10) RIGHT SIDE XL EXIT	n/a	12) LEFT SIDE XL ENTRANCE	n/a
Technician name: [redacted]		Date: 3 / 1 / 2011	
Meter Manufacturer and Model: ThermoFisher RadEye PRD		Unit Model and Serial Number: CT-80DR 40614	
Meter Serial Number: 14528		Unit Location: MAF	
Meter Calibration Due Date: July 9, 2011		Background: 4	
Notes (Reason for Survey): Annual PM			