REVEAL

[redacted]

[redacted]

DOC NO: 40009 Rev: D

TITLE: RADIATION SURVEY MAP FOR
CT-80, CT-80XL, CT-80DR, & CT-80DRXL
RADIATION LIMIT: < 400 µR/hr
All Readings in µR/hr unless otherwise stated

CT-80 / CT-80DR

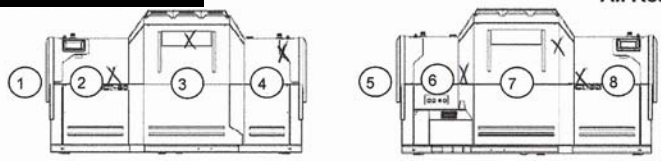

CT-80XL / CT-80DRXL

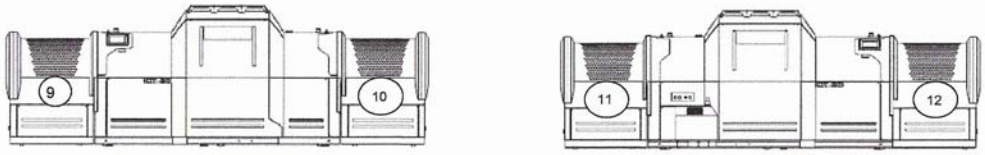

TEST RECORD

ZONE	RADIATION LEVEL VALUE (< 400 µR/hr)	ZONE	RADIATION LEVEL VALUE (< 400 µR/hr)
1) ENTRANCE END	115 uR/hr	5) EXIT END	70 uR/hr
2) RIGHT SIDE ENTRANCE TUNNEL	4 uR/hr	6) LEFT SIDE EXIT TUNNEL	3 uR/hr
3) RIGHT SIDE GANTRY	15 uR/hr	7) LEFT SIDE GANTRY	4 uR/hr
4) RIGHT SIDE EXIT TUNNEL	3 uR/hr	8) LEFT SIDE ENTRANCE TUNNEL	3 uR/hr
9) RIGHT SIDE XL ENTRANCE	N/A	11) LEFT SIDE XL EXIT	N/A
10) RIGHT SIDE XL EXIT	N/A	12) LEFT SIDE XL ENTRANCE	N/A
Technician name: [redacted]		Date: 3/10/2011	
Meter Manufacturer and Model: Thermo Rad Eye PRD		Unit Model and Serial Number: CT80, 040040	
Meter Serial Number: 14526		Unit Location: MCI	
Meter Calibration Due Date: 9 July 2011		Background: 3 uR/hr	
Notes (Reason for Survey): Annual PM			